


Medtrica Tip Protector TIP550100; TIP650100 Instructions for Use



1. Slide the **smaller** end of the tip protector over the end of the medical instrument that requires protection immediately **after** high heat **or before** low temperature and/or chemical based reprocessing.
 2. Allow 20 – 30% of the **larger** end of the tip protector to overhang the end of the medical instrument.
 3. Remove the tip protector just before the procedure. Final prep the instrument.
 4. At completion of the procedure, perform bedside pre-cleaning and then **put the same tip protector back on the instrument before transport.**
 5. Do not remove the tip protector during transport and initial manual cleaning.
 6. Before the end of manual cleaning, remove and dispose of the tip protector and complete the manual cleaning of the instrument tip - (manual clean where the tip protector was).
- **For use during pre-cleaning, manual cleaning, transport & storage**
 - **Designed for one-time usage**

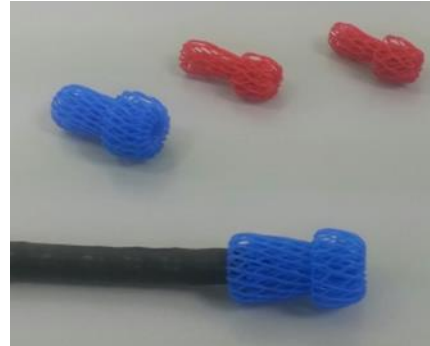

Tip protectors are expandable:

Small / Red: for instruments that are approximately 2mm to 10mm

Large / Blue: for instruments that are approximately 7mm to 15mm

Description:

- Clean, non-absorbing, semi-rigid expandable mesh protects the tip of sensitive medical instruments from front and side impact
- Allows for airflow and moisture to escape, eliminating potential bacteria growth (Pseudomonas species) that is possible with other tip protectors
- Will not fall off and is not abrasive/will not scratch any part of the instrument/lens

Specifications:

Tip protector is Clean, Non-sterile, Latex free, Non-absorbable material; Max Temp 79° C